





### Features

- Differential pressure transmitter with linear curve for air-conditioning applications
- · Also available as a two-wire system ("PIZ" model)
- · Also for ± measurement ranges and asymmetric measurement ranges
- · With optional LCD
- · suitable for wall mounting



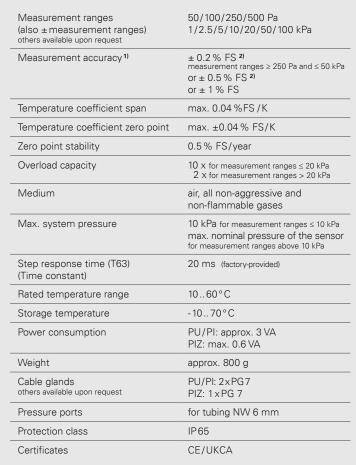

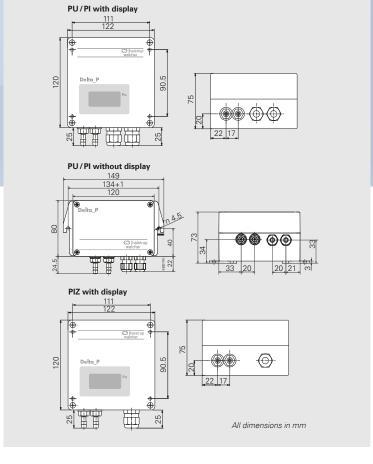

Order code	Α	В	С	D	E	F	G
	-	-	-	-	-	-	_

Model	Output signal	Α
PU	$010V\left(R_{_{L}}\geq2k\Omega\right)$	U
PI	$020 \text{ mA} (R_{L} \leq 500 \Omega)$	10
PI	$420 \text{ mA } (R_{\scriptscriptstyle L} \leq 500 \Omega)$	14
PIZ	420 mA two-wire (R <sub>1</sub> ≤ 50 [U <sub>R</sub> (V)-10 (V)]Ω)	ΙZ

Measurement range	В
Measurement range e.g. 0 100 Pa, 0 60 mbar, ±110 mmHg (etc.)	

Measurement accuracy	С
$\pm$ 0.2 % FS <sup>2)</sup> only for measurement ranges $\geq$ 250 Pa and $\leq$ 50 kPa	02
± 0.5 % FS <sup>2)</sup>	05
± 1 % FS	1

2) not for PIZ with ± measurement ranges

Supply voltage	D
24 VDC, +20 %/-15 % <sup>3)</sup>	24D
24 VAC, ±10 % <sup>3)</sup> (with galvanic isolation)	24A
115 VAC, ±10 % <sup>3)</sup>	115
230 VAC, ±10%³)	230
1032 V DC (two-wire system) 4)	PIZ

- 3) not for PIZ
- 4) only for PIZ

Step response time	E
none	0
1s	1
2s	2
5s	5

LCD	F
none	0
3 ½ digits (see foto)	3
4½ digits (only for PU/PI)	4

Calibration certificate	G
none	0
Factory calibration	- 1
Calibration according to DKD-R 6-1	D

# **Accessories and software**

# **Accessories**

Connection parts	Order no.
Silicone tubing ID 5 mm, AD 9 mm, red (please state length required)	9601.0003
Silicone tubing ID 5 mm, AD 9 mm, blue (please state length required)	9601.0004
Norprene tubing ID 4,8 mm, AD 8 mm, black (please state length required)	9061.0002
Y-piece for tubing, NW 5mm	9601.0171

#### **Pressure connections**

You can also obtain numerous customized pressure connections from us, e.g. various cutting ring fittings or hose nozzles.




## **Application software**

You can set the parameters for our instruments or monitor and record measurements using a PC via a USB or RS232 interface. These features are supported by our free user software. This also allows you to transfer your settings to other devices by saving and reusing them.

Our user software is compatible with the following pressure transmitters: P 26, P 34 and P 29.

You can download the software here:

www.halstrup-walcher.de/en/software

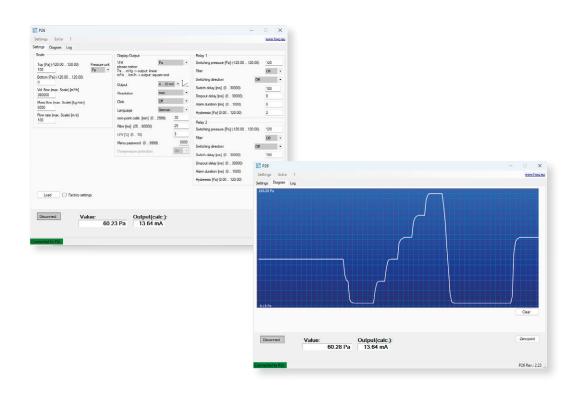

### **Calibration services**

You can also have our devices tested and confirmed in our accredited calibration laboratory in accordance with DKD-R 6-1 or as a factory calibration. Our trained experts will be happy to advise you on the calibration of

our pressure measurement devices. Recalibration of third-party devices that are included in our scope of accreditation is also possible. If required, we offer adjustment for pressure measurement products manufactured by halstrup-walcher. In addition, we offer you further services within the scope of calibration, please contact us.

You can find more information at: www.halstrup-walcher.de/en/products/calibration.php

